


# ILLUSTRATION DRAWING REFERENCE ONLY

REVISIONS			
REV.	DESCRIPTION	DATE	APPROVED
A	SEE ECN 9159	8/7/09	MCS

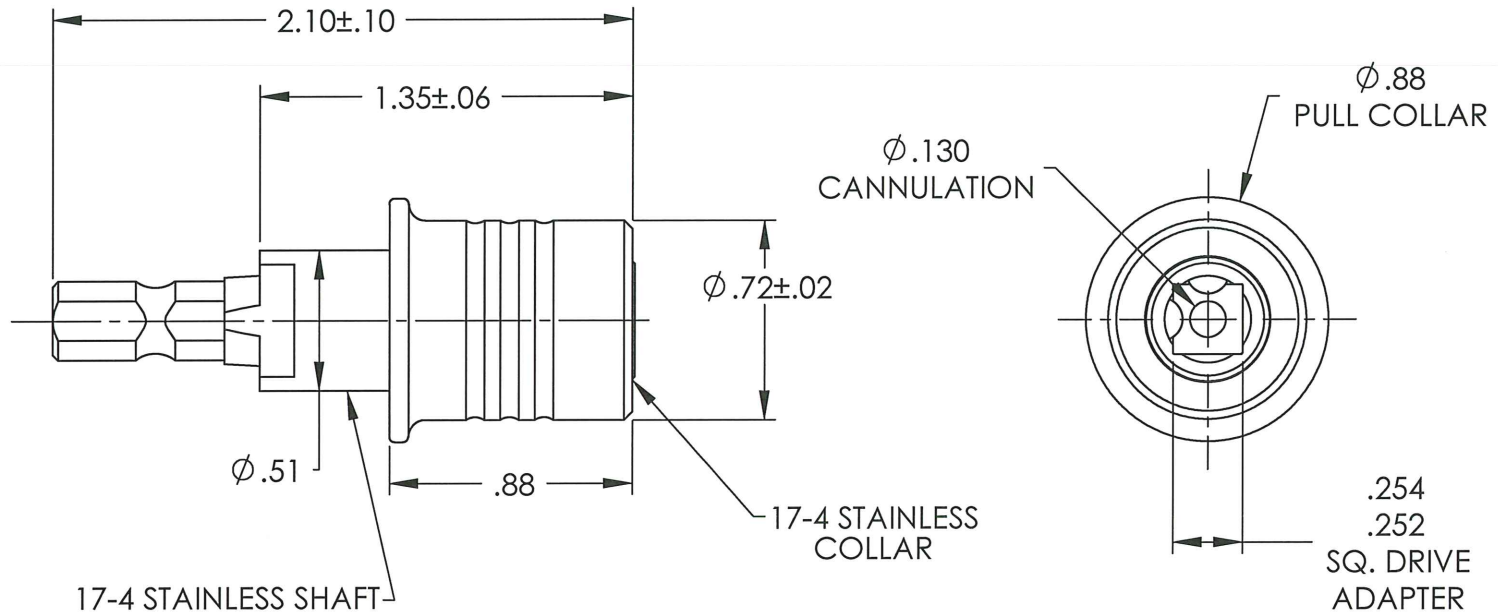

## CUSTOMER APPROVAL

APPROVED BY: \_\_\_\_\_

DATE: \_\_\_\_\_

THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF GAUTHIER BIOMEDICAL, INC., ANY REPRODUCTION IN PART OR WHOLE WITHOUT THE WRITTEN PERMISSION OF GAUTHIER BIOMEDICAL, INC. IS PROHIBITED.

### INSPECTION SYMBOLS

-  CRITICAL
-  AQL

UNLESS OTHERWISE SPECIFIED  
DIMENSIONS ARE IN INCHES  
TOLERANCES ARE:  
FRACTIONS DECIMALS ANGLES  
±1/32 .X ±.020 ±1°  
.XX ±.010  
.XXX ±.005  
.XXXX ±.0005



Gauthier Biomedical Inc.

GAUTHIER BIOMEDICAL, INC.  
1235 NORTH DAKOTA DRIVE, SUITE G  
GRAFTON, WI 53024  
(262) 546-0010 ph. (262) 546-0011 fax  
E-mail: engineering@gauthierbiomedical.com

MATERIAL SEE DETAILS	APPROVALS	DATE
HEAT TREAT	DRAWN RJB	7/2/09
FINISH	CHECKED RJB	8/11/09
PASSIVATE	APPROVED RJB	8/11/09
	DO NOT SCALE DRAWING	
	ANODIZE	

DESCRIPTION		
1/4" SQ. QUICK CONNECT W/MALE TRINKLE,		
SIZE	PART NUMBER	REV.
A	GA100509	A
SCALE 2:1	CAD FILE: GA100509	SHEET 1 OF 1